



TiO₂ nanotubes as solid-phase extraction adsorbent for the determination of polycyclic aromatic hydrocarbons in environmental water samples

Bochra Bejaoui Kefi¹, Latifa Latrous El Atrache^{2,*}, Hafedh Kochkar¹, Abdelhamid Ghorbel³

1. Laboratoire des Matériaux Utiles, Institut National de Recherche et d'Analyse Physico-chimique, pôle technologique Sidi-Thabet 2020 Tunis, Tunisia

2. Laboratoire de Chimie Analytique et Electrochimie, Département de Chimie, Faculté des Sciences de Tunis, Campus Universitaire, 2092 EL Manar Tunis, Tunisia. E-mail: latrous.latifa@topnet.tn

3. Laboratoire de Chimie des Matériaux et Catalyse, Faculté des Sciences de Tunis, Campus Universitaire, 2092 EL Manar Tunis, Tunisia

Received 13 May 2010; revised 02 September 2010; accepted 12 September 2010

Abstract

An analytical method based on TiO₂ nanotubes solid-phase extraction (SPE) combined with gas chromatography (GC) was established for the analysis of seven polycyclic aromatic hydrocarbons (PAHs): acenaphthylene, acenaphthene, anthracene, fluorene, phenanthrene, fluoranthene and pyrene. Factors affecting the extraction efficiency including the eluent type and its volume, adsorbent amount, sample volume, sample pH and sample flow rate were optimized. The characteristic data of analytical performance were determined to investigate the sensitivity and precision of the method. Under the optimized extraction conditions, the method showed good linearity in the range of 0.01–0.8 µg/mL, repeatability of the extraction (RSD were between 6.7% and 13.5%, $n = 5$) and satisfactory detection limits (0.017–0.059 ng/mL). The developed method was successfully applied to the analysis of surface water (tap, river and dam) samples. The recoveries of PAHs spiked in environmental water samples ranged from 90% to 100%. All the results indicated the potential application of titanate nanotubes as solid-phase extraction adsorbents to pre-treat water samples.

Key words: TiO₂ nanotubes; hydrothermal treatment; solid phase extraction; gas chromatography; polycyclic aromatic hydrocarbons

DOI: 10.1016/S1001-0742(10)60481-0

Citation: Bejaoui Kefi B, Latrous El Atrache L, Kochkar H, Ghorbel A, 2011. TiO₂ nanotubes as solid-phase extraction adsorbent for the determination of polycyclic aromatic hydrocarbons in environmental water samples. *Journal of Environmental Sciences*, 23(5): 860–867

Introduction

Polycyclic aromatic hydrocarbons (PAHs) are widespread contaminants throughout the environment and originate mainly from anthropogenic sources such as the combustion of fossil fuels and the direct release of oil products (Poster et al., 2006). They present an important class of organic contaminants, and many of them with four or more rings are carcinogenic and mutagenic because of their metabolic transformation capacities (Li et al., 2001; ATSDR, 1995). Due to the extensive amount of data suggesting the hazards of these compounds, the European Water Framework Directive (WFD) establishing a list of six PAHs priority substances (anthracene, benzo[a]pyrene, benzo[b]fluoranthene, benzo[k]fluoranthene, benzo[g,h,i]perylene, ideno[1,2,3-cd]pyrene) are classified as priority hazardous substances, and naphthalene, as well as fluoranthene as priority substances (Directive 2000/60/EC; Decision No 2455/2001/EC).

International standardised methods for analysing PAHs

in surface waters are available, including ISO 17993 method based on high-performance liquid chromatography (HPLC) with fluorescence detection after liquid-liquid extraction, and ISO/CD 28540 method based on gas chromatography–mass spectrometry after either liquid-liquid or solid phase extractions. EPA method 525.1 using C18 silica adsorbent for PAH extraction, is also widely used.

Solid phase extraction (SPE) is a well-established technique for the extraction of various pollutant species at low concentration level. This technique is extinguished from the liquid-liquid extraction because of its advantages of high recovery, high enrichment factor, short extraction time, and low consumption of organic solvents. Recently, carbon nanotubes divided into single-walled carbon nanotubes and multi-walled carbon nanotubes (MWCNT) (Cai et al., 2003a, 2003b, 2005; Yang and Xing, 2006; Yang et al., 2006a, 2006b) have attracted more attention as SPE adsorbent. Wang et al. (2007) used MWCNT as adsorbent for solid-phase extraction of PAHs in environmental waters. Moreover, many nanotubes materials have been synthesised such as: titanium dioxide (TiO₂),

* Corresponding author. E-mail: latrous.latifa@topnet.tn

zirconium dioxide, silica, V₂O₅, MoO₃ (Liu et al., 2007; Mor et al., 2006; Jung et al., 2002). It is reported that TiO₂ nanotubes have larger surface area than the starting titanium, and contain more ion-exchangeable OH groups in the interlayer and surface (Kasuga, 2006; Liu et al., 2005). TiO₂ nanotubes has also gained great interests in analytical chemistry because of its high chemical stability, durability, corrosion resistance, non toxicity and cost effectiveness. Micro-scaled TiO₂ has been used as stationary phase in HPLC applications (Nawrocki et al., 2004) as well as a solid phase extraction adsorbent for the enrichment of metal ions (Vassileva et al., 1996; Camel, 2003; Zhang et al., 2005) and selective extraction of phosphates (Kawahara et al., 1989; Matsuda et al., 1991; Ikeguchi and Nakamura, 1998), phospholipids (Ikeguchi and Nakamura, 1999, 2000) and phosphopeptides (Sano and Nakamura, 2004a, 2004b; Pinkse et al., 2004). TiO₂ nanotubes were demonstrated to be excellent adsorbents of inorganic cations and anions as well as organic compound (Diebold 2004; Liang et al., 2001; Li et al., 2004; Li and Deng, 2002; Chen and Chen, 2005). Zhou et al. (2007) investigated the feasibility of TiO₂ nanotubes as SPE adsorbent for the extraction of dichlorophenyltrichloroethane (DDT) and their metabolites in environmental water samples.

However, there was no literature about application of TiO₂ nanotubes to the enrichment of PAHs from environmental water samples. In the present work, we demonstrated for the first time the applicability of TiO₂ nanotubes as SPE adsorbent. We investigated the selective separation of acenaphthene, acenaphthylene, anthracene, fluorene, phenanthrene, fluoranthene and pyrene (cited among the 16 PAHs considered as priority by the EPA) as PAHs model compounds. Factors that may influence the enrichment efficiencies of the target PAHs (kind and volume of eluent, sample flow rate, sample pH, sample volume and adsorbent amount) were optimised. Furthermore, efficiency of the TiO₂ nanotubes as adsorbent for the enrichment of selected PAHs at trace levels in tap and surface waters was investigated.

1 Experimental

1.1 Reagents

Organic solvents, acetonitrile (ACN), methanol, dichloromethane (DCM) and hexane were of the HPLC grade. Ultra pure water was prepared in the laboratory using a Milli-Q system (Millipore, Elix, France). Certified PAHs reference standards acenaphthene (Ace), acenaphthylene (Acy), anthracene (Ant), fluorene (Flo), phenanthrene (Phn), fluoranthene (Flr) and pyrene (Pyr) were purchased from Sigma-Aldrich (USA). These standards were dissolved in DCM at 0.1 µg/mL. Stock solutions were protected from light and stored at 4°C. Working solutions were prepared daily by an appropriate dilution of the stock solutions with methanol.

Titanium dioxide (68% anatase and 32% rutile, P25, Degussa-Hüls AG); sodium hydroxide (Fisher Chemicals, UK), and hydrochloric acid (Panreac Quimica SA, Spain)

were used without further purification.

Acetate buffer solution (CH₃COO⁻/CH₃COOH) was prepared by mixing appropriate volumes of 0.1 mol/L acetic acid and 0.1 mol/L sodium acetate solutions at pH 4. Ammonium buffer solution was prepared by mixing appropriate amounts of 0.1 mol/L ammonia and 0.1 mol/L ammonium chloride solutions at pH 9.

1.2 Materials characterization

The N₂ adsorption-desorption isotherms at 77 K were performed using a Micromeritics ASAP 2000 analyzer (USA). The Brunauer-Emmett-Teller (BET) equation was used to calculate the specific surface area (*S*_{BET}). Mean pore diameter (*d*_p) was obtained using the Barrett-Joyner-Halenda (BJH) model in the range of mesopores. X-ray diffraction (XRD) patterns were obtained by a PANalytical X'Pert Pro (the Netherlands) apparatus using CuKα radiation ($\lambda = 1.542 \text{ \AA}$) for investigating the crystallization behaviour. Low magnification TEM images were taken at an accelerating voltage of 200 kV on a JEOL-2010 (Japan) instrument. HRTEM images were taken at an accelerating voltage of 400 kV. Specimens for the TEM studies were prepared by depositing a drop of aqueous suspension of the samples onto 300 mesh Cu grid, coated with a lacey carbon film.

PAHs were analyzed using an Agilent 6890N Network GC System (USA) with flame ionization detector (FID). An HP-5MS column coated with 5% phenyl methylsiloxane (30 m × 0.25 mm, with 0.25 µm film thickness) was used for separation of studied compounds. Helium (1 mL/min) was used as carrier gas. The GC oven temperature was kept at 50°C for 2 min and programmed to 250°C at a rate of 8°C/min. The split ratio was adjusted at 1:10 and the injector temperature was maintained at 250°C. The FID detector temperature was kept at 300°C.

1.3 Preparation of titanate nanotubes

The alkaline hydrothermal method, as described by Kochkar et al. (2009) was used to prepare the titanate nanotubes. Specifically, a commercial TiO₂ (0.50 g) was dispersed in a 15 mL aqueous solution of 11.25 mol/L NaOH and placed into a teflon-lined autoclave with an 80% filling factor. The autoclave was then heated at 403 K for 20 hr to prepare the hydrogenotitanate nanotubes (HNTs) samples. A white precipitate was isolated upon filtration and washed repeatedly with 1000 mL of hot ultra pure water until the supernatant pH value attained 9. In a second step, an aqueous solution containing the precipitate was neutralized using a 0.1 mol/L HCl solution until a pH value of 7 was reached. The precipitate was then subsequently washed with 500 mL ultra pure water to remove NaCl formed in excess. The obtained wet solids were dried in an oven at 353 K for 24 hr. Finally, HNTs nanotubes were calcined at 773 K under air for 2 hr.

1.4 SPE procedure

TiO₂ nanotubes packed cartridges were prepared by modifying an Agilent ZORBAX SPE C18 cartridge (0.2 g, 3 mL, polypropylene). The C18 packing was evacuated,

and 0.1 g TiO₂ nanotubes were packed in the cartridge. The polypropylene upper and lower frits remained at each end of the cartridge to hold their packing TiO₂ nanotubes in place. The packed cartridge was placed in a vacuum elution apparatus. This solid phase was first conditioned with 10 mL of methanol and 10 mL of deionised water. Then a known volume of ultra pure water or sample water spiked with the seven target analytes was applied to the column. After that, the retained PAHs were eluted with an optimum volume of DCM and finally the extract was dried to 1 mL with nitrogen gas in water bath at 35°C.

1.5 Water samples

Tap water and surface water samples were selected for validating the proposed method. Tap water sample was collected from our own laboratory after it was flowing for 10 min at very large rate. However, dam water samples were obtained from Sidi Salem and Sejnene reservoirs. All the collected water samples were filtered through a Millipore membrane with pore size 0.45 µm immediately after sampling and were maintained in amber glass bottles at 4°C. To avoid PAHs adsorption in the glass of bottles, samples were rapidly extracted.

2 Results and discussion

2.1 TiO₂ nanotubes characterization

The change in the crystal structure from the starting P25 powder to one dimensional titanate structures was studied by XRD. All peaks in the XRD patterns (Fig. 1) were assigned to the H₂Ti₂O₅·H₂O, which showed an orthorhombic system with the lattice constants $a_0 = 1.926$ nm, $b_0 = 0.378$ nm and $c_0 = 0.300$ nm (Yang et al., 2003). Up-on calcination of TiO₂ nanotubes at 773 K, it can be seen from Fig. 1, that the intensity of the diffraction peak (110) near $2\theta \approx 30^\circ$ was decreased and shifted towards a higher angle value, indicating a decrease in the interlayer distance in this plane. This contraction of layers may be due to the release of water molecules adsorbed and presented in the spacing. New peaks appeared showing the transformation of the initial HNT sample to anatase phase.

The effect of calcination temperature on the pore size distribution, mesoporous volume and surface area has been investigated and the results are illustrated in Table 1. For temperature > 403 K, the surface area was found to be strongly influenced by the calcination temperatures; it decreases to 99 m²/g at 773 K, indicating sintering of the nanotubes. However, the pore distribution increases due to the aggregation of formed nanoparticles. The drop in surface area and mesoporous volume is in accordance with previous observations by Edison et al. (2006) for Na_xH_{2-x}Ti₃O₇.

Changes in the morphology of the nanotubes occurring with respect to temperature were followed using TEM analysis. Figure 2 shows transmission electron micrographs of the starting material as well as after calcination at 773 K for 2 hr. It can be seen from fig. 2a that the initial material is quite homogeneous with a large number

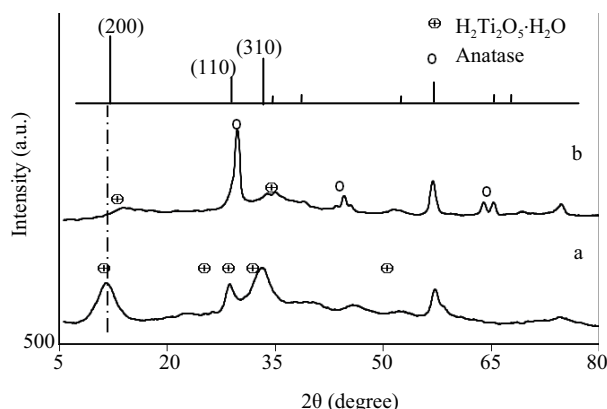


Fig. 1 XRD patterns of titanate nanotubes support (line a) and comparison with the expected XRD peak intensities of the H₂Ti₂O₅ phase (line b) after calcination at 773 K.

Table 1 Textural properties of TiO₂ nanotubes

Temperature (K)	S_{BET} (m ² /g)	V_p (cm ³ /g)	d_p (nm)
403	269	0.67	9
773	99	0.63	23

S_{BET} : BET surface area; V_p : porous volume; d_p : mean pore diameter.

of nanotubes. The outer diameters of tubes were 6–8 nm and inner diameters were 4–6 nm, and the lengths were measured to be several hundreds of nanometres. All the tubes were open at both ends. The HRTEM analysis shows that the walls of the nanotubes were amorphous (Fig. 2b). The morphology of the nanotubes remained hardly affected up to 773 K even the outer and inner diameters decrease to 7–5 nm (Fig. 2c). However, HRTEM analysis showed that the initially amorphous nanotubes walls were transformed into crystalline anatase (Fig. 2d). This was also consistent with the XRD results showing that the patterns drastically changed after calcination at 773°C.

Nanotubes were successfully obtained directly from TiO₂ (P25) following a hydrothermal process in the presence of sodium hydroxide. The nanotubes retained their morphology up to 773 K. Only a change in the structure related to the transformation of orthorhombic HNTs into anatase TiO₂ was observed.

The anatase TiO₂ nanotubes were used as adsorbent for the SPE of PAHs at trace levels in water samples. There are many factors that may influence the enrichment efficiencies of the PAHs compounds such as the kind of elution solvent and its volume, the sample volume, the sample pH, the sample flow rate and the mass of adsorbent. To determine optimum factors that ensure the entire recovery of all the analytes adsorbed, Milli-Q water was spiked with the seven PAHs compounds at 0.1 µg/mL concentration level.

2.2 Effect of elution solvent

To ensure the completely elution of the target PAHs from the cartridge, an optimum solvent polarity should be chosen. For this purpose, four solvents with different polarities were tested: hexane < DCM < acetonitrile < methanol. Elution of PAHs from cartridge was performed

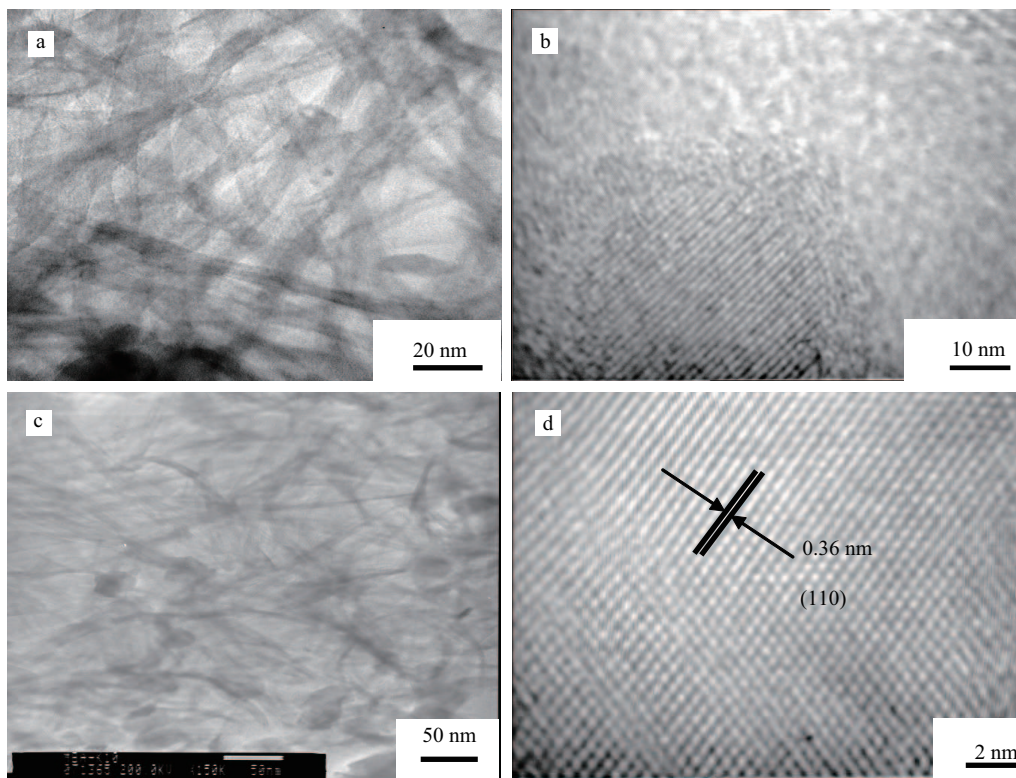


Fig. 2 TEM (a) and HRTEM (b) images of H₂Ti₂O₅·H₂O; TEM (c) and HRTEM (d) images after calcination at 773 K.

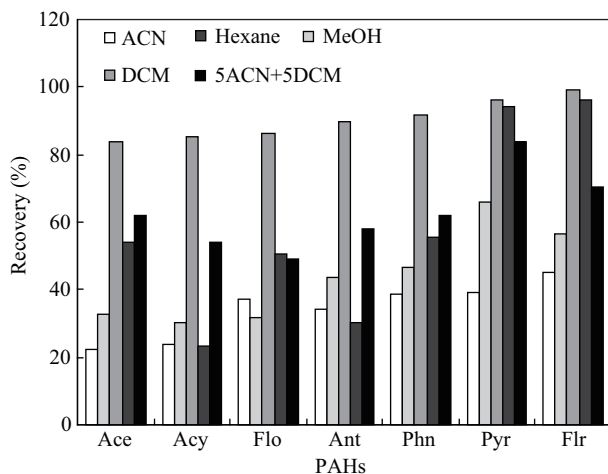


Fig. 3 Influence of elution solvent on analytes recovery. Spiked sample concentration: 0.1 µg/mL for each compound; eluent volume: 10 mL; sample flow rate: 3 mL/min; sample pH: 6 and sample volume: 100 mL. ACN: acetonitrile; MeOH: methanol; DCM: dichloromethane.

with 10 mL of the selected organic solvent. An intermediate solvent polarity was obtained by mixing acetonitrile and DCM (5:5, V/V). It seems clear that the recovery of PAHs compounds is related to the solvent polarity (Fig. 3). This is due to different partition constants of PAHs between TiO₂ nanotubes (solid phase) and solvent (liquid phase). The experimental results demonstrated that DCM, with a medium polarity, gave the much high elution efficiency than other organic solvents for all of the target analytes, therefore it was selected as the elution solvent for the next optimisation steps.

The volume of the eluent has an great effect on the elution performance and efficiency. To find out the required DCM volume to recover all the analytes from TiO₂

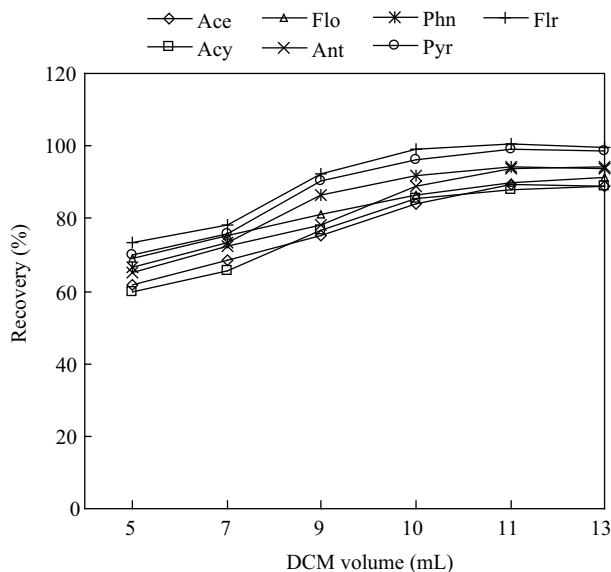


Fig. 4 Effect of eluent volume on analyte recoveries. Other conditions are the same as in Fig. 3.

nanotubes packed cartridge, eluent volumes in the range of 5–13 mL were tested. From Fig. 4, it suggested that PAHs compounds needed a volume of eluent more than 11 mL to get the best recoveries. Thus, to achieve complete elution of the seven analytes, 12 mL DCM was utilized in following experiments.

2.3 Effect of sample flow rate

The influence of sample flow rate was investigated over the range of 1–8 mL/min with the other conditions kept constant. The experimental results shown in Fig. 5 indicated that 3 mL/min was optimal flow rate which was

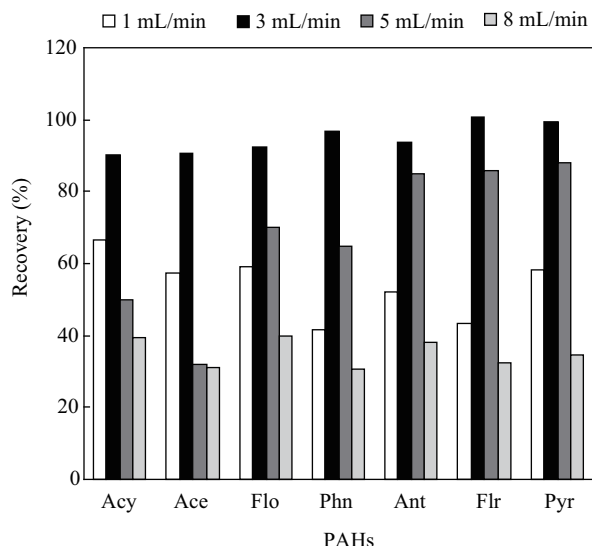


Fig. 5 Effect of the sample flow rates on PAHs recoveries. Eluent: 12 mL DCM; other conditions were same as in Fig. 3.

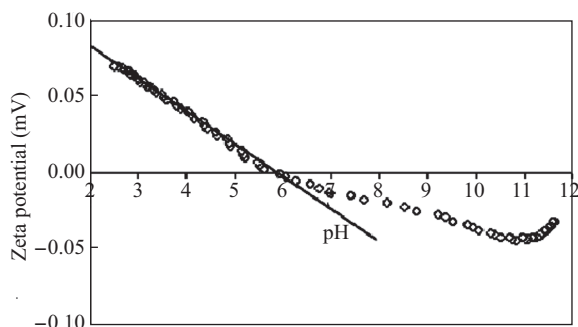


Fig. 6 Zeta potential values of TiO₂ nanotubes as a function of solution pH.

selected for further use in the following experiment.

2.4 Effect of sample pH

Sample pH plays an important role in the SPE procedure and affects the extraction efficiency. pH factor determine the surface charge of the TiO₂ nanotubes. The OH group can be protonated in acidic solution then TiO₂ nanotubes have positive surface charge. However, in alkaline media the OH group can be deprotonated and they have negative surface charge. The effect of sample pH on the recoveries of selected PAHs was examined in a range of 4–9. For most of objectives satisfactory recoveries were obtained at pH 6 (Fig. 6). This result is in agreement with that of Zhou et al. (2007) who studied the feasibility of TiO₂ nanotubes for the enrichment of the DDT and its metabolites in environmental water samples. Zeta potential (ZP) of titanium nanotubes as function of solution pH was determined (with zetalyzer 2000 apparatus). Figure 6 shows the ZP-pH curve of the TiO₂ in aqueous media (1 g/L). Three different surface charges (positive, zero, and negative) were detected, depending on the solution pH. The zero zeta potential (pH between 5.5 and 6) coincides with the sample pH allowing maximum extraction recoveries.

2.5 Effect of sample volume

In order to obtain reliable and reproducible analytical results and satisfactory recoveries for all the studied compounds, the breakthrough volume in the solid phase extraction was investigated. Different volumes (100–500 mL) of ultra pure water spiked with 0.1 µg/mL of each PAH analytes were preconcentrated by TiO₂ nanotubes packed cartridges. As described in Fig. 7, recovery levels obtained for studied PAHs decrease when the treated water volume increases from 100 to 400 mL. Based on these results, the sample volume of 100 mL was selected in the subsequent analysis.

2.6 Effect of amount of cartridge packing

The efficiency of the TiO₂ nanotubes amount on the recovery of analytes was studied. Three solid phase amounts were tested (100, 200 and 300 mg) for the preconcentration of PAH compounds in spiked Milli-Q water. Obtained results (Fig. 8) showed insignificant differences in recoveries among the different amounts of cartridge packing. Therefore, the TiO₂ nanotubes amount of 100 mg was recommended for the extraction of PAHs compounds.

2.7 Characteristics of the method

For the precision of this method, five replicate samples spiked at 0.1 µg/mL were carried out using the optimum conditions described above. The recoveries of Acy, Ace, Flo, Ant, Phn, Pyr and Flr were 90.2%, 90.8%, 92.2%, 93.9%, 97.0%, 99.5% and 100.9% respectively. The relative standard deviations (RSD) were 7.3% for Acy, 12.4 for Ace, 6.7 for Flo, 6.8 for Phn, 11.2 for Ant, 13.0 for Flr and 13.4 for Pyr. As a new adsorbent for SPE, TiO₂ nanotubes present some limitation in terms of stability and repeatability (RSD > 5%), this can be improved by enlarging the surface area and controlling the pore size.

Under the conditions selected above, calibration graphs were linear in the range of 0.01–0.80 µg/mL for each PAH compounds. Calibration equations, correlation coefficient as well as the detection limit ($S/N = 3$) of each analyte are illustrated in Table 2. TiO₂ nanotubes, as SPE adsorbent,

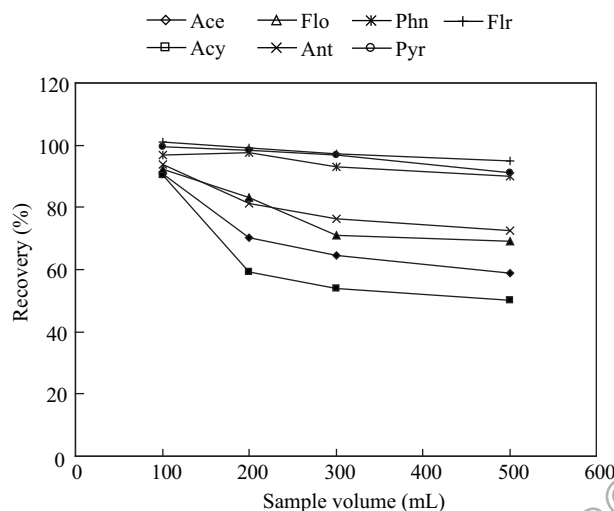


Fig. 7 Effect of sample volume on PAHs recoveries. Conditions are the same as in Fig. 5.

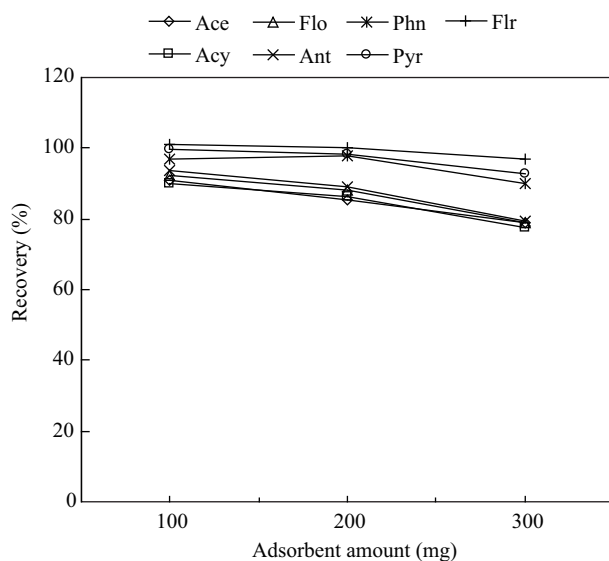


Fig. 8 Effect of TiO₂ nanotubes amount on the PAHs recoveries. Conditions are the same as in Fig. 7.

provided reproducible and reliable analytical results and showed good linear correlation $R^2 \geq 0.994$.

2.8 Comparison study

The present results with TiO₂ nanotubes, as new sorbent for the SPE, were compared to traditional method using C18 silica sorbent. PAHs were extracted from water samples by C18 procedure as described by Oleszczuk and Stanisław (2004). Results were also compared to that presented by Wang et al. (2007) using MWCNTs sorbent. Figure 9 shows that TiO₂ nanotubes presented its comparable adsorbent properties to MWCNTs but superior to C18. The three SPE procedures applied to PAHs presented competitive results. But sometimes it is necessary to take into account the cost of adsorbent in addition to its analytical performance. However, MWCNTs and C18

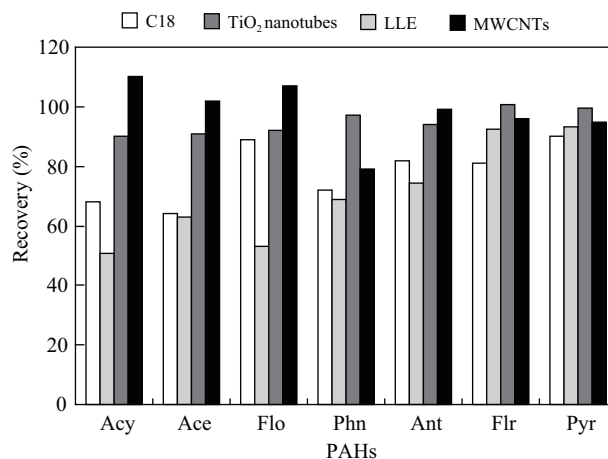


Fig. 9 Extraction recoveries obtained with C18, MWCNTs and TiO₂ nanotubes sorbents and with liquid-liquid extraction.

silica sorbents are more expensive than the TiO₂ nanotubes elaborated with the simple hydrothermally method.

Liquid-liquid extraction (LLE) of PAHs from water samples was done as described by Brum et al. (2008) and experimental results were compared to that obtained with TiO₂ nanotubes sorbent. According to the results shown in Fig. 9, the difference of recoveries between the two extraction procedures was important with the exception of Flr and Pyr cases. SPE method presents more advantages than LLE especially when using nanoscaled materials as sorbents. Indeed, their strong adsorption affinity to a wide variety of organic compounds, together with their large adsorption surface make them excellent material for SPE.

2.9 Application to environmental water samples

In order to investigate the feasibility of TiO₂ nanotubes in the application of environmental sample analysis, all retained SPE conditions were assessed on real spiked water samples (tap, river and dam waters). Firstly, blanks of

Table 2 Calibration equation, correlation coefficient and the detection limit of each PAH analyte

Compound	Linear range (µg/mL)	Calibration equation	R ²	Detection limit* (ng/mL)
Acy	0.01–0.50	$y = 1.6690x - 10^{-4}$	0.9999	0.031
Ace	0.05–0.40	$y = 1.8504x - 10^{-4}$	0.9998	0.017
Flo	0.05–0.40	$y = 1.2195x - 10^{-4}$	0.9971	0.026
Phn	0.05–0.80	$y = 2.2420x + 3 \times 10^{-4}$	0.9997	0.053
Ant	0.05–0.80	$y = 1.3812x - 2 \times 10^{-4}$	0.9982	0.015
Flr	0.05–0.40	$y = 2.5889x - 3 \times 10^{-5}$	0.9944	0.017
Pyr	0.01–0.80	$y = 1.8366x - 8 \times 10^{-5}$	0.9959	0.059

* Detection limits were calculated using $S/N = 3$.

Table 3 Recovery percentages of tap and surface water samples spiked at two concentrations levels

Compound	Recovery of tap water (%)		Recovery of surface water (%)			
	0.05 µg/mL	0.1 µg/mL	Sidi Salem		Sejnane	
			0.05 µg/mL	0.1 µg/mL	0.05 µg/mL	0.1 µg/mL
Acy	85.4	93.3	82.4	84.3	85.0	88.4
Ace	83.4	94.1	87.5	90.3	81.7	88.5
Flo	86.2	94.9	89.2	91.1	87.3	90.3
Phn	88.9	97.2	88.8	94.5	91.0	93.8
Ant	85.5	93.0	88.1	90.7	89.3	89.5
Flr	94.3	99.5	93.5	97.6	90.5	96.2
Pyr	92.6	98.4	90.5	96.7	89.7	94.9

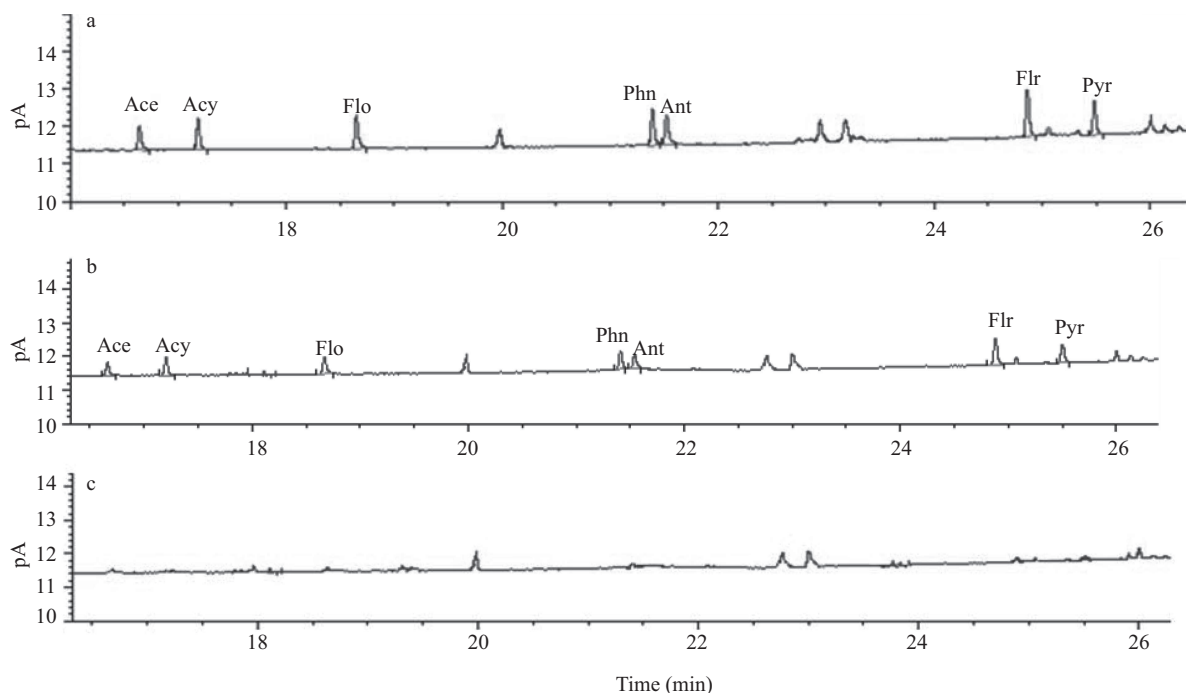


Fig. 10 Chromatograms of surface water samples. (a) blank of tap water, (b) tap water sample spiked with 0.05 µg/mL of each compound, and (c) tap water sample spiked with 0.1 µg/mL of each compound. Eluent: DCM; 12 mL; sample flow rate: 3 mL/min; sample pH: 6; sample volume: 100 mL and TiO₂ nanotubes amount: 100 mg.

all samples were run then 100 mL waters spiked at 0.05 and 0.1 µg/mL were passed through the SPE cartridge. The analytical results of the proposed method are given in Table 3 and the chromatograms of the blank and spiked tap waters are exhibited in Fig. 10. Using this method, little matrix effect was found for the SPE of PAHs. The recoveries obtained were between 81.7% and 99.5%.

3 Conclusions

In this study, a simple, efficient and reliable method was set up to determine PAHs in the aqueous solution using titanate nanotubes as SPE sorbent coupled with GC. According to our experimental results, titanate nanotubes packed cartridge has good analytical potential for the extraction of some PAHs compounds such as acenaphthene, acenaphthylene, anthracene, fluorene, phenanthrene, fluoranthene and pyrene from real environmental water samples. Taking into account the simplicity and low cost of TiO₂ nanotubes elaboration, as well as the good extraction efficiencies, this nanostructured titania has great potential of becoming a cost effective and useful extraction tool in analytical methods.

References

ATSDR (Agency for Toxic Substances and Disease Registry), 1995. Toxicological Profile for Polycyclic Aromatic Hydrocarbons. US Department of Health and Human Services Atlanta.

Brum D M, Cassella R J, Pereira Netto D A, 2008. Multivariate optimization of a liquid-liquid extraction of the EPA-PAHs from natural contaminated waters prior to determination by

liquid chromatography with fluorescence detection. *Talanta*, 74: 1392–1399.

- Cai Y, Jiang G, Liu J, Zhou Q, 2003a. Multiwalled carbon nanotubes as a solid-phase extraction adsorbent for the determination of bisphenol A, 4-*n*-nonylphenol, and 4-*tert*-octylphenol. *Analytical Chemistry*, 75: 2517–2521.
- Cai Y, Jiang G, Liu J, Zhou Q, 2003b. Multi-walled carbon nanotubes packed cartridge for the solid-phase extraction of several phthalate esters from water samples and their determination by high performance liquid chromatography. *Analytica Chimica Acta*, 494: 149–156.
- Cai Y, Mou S, Lu Y, 2005. Multi-walled carbon nanotubes as a solid-phase extraction adsorbent for the determination of chlorophenols in environmental water samples. *Journal of Chromatography A*, 1081: 245–247.
- Camel V, 2003. Solid phase extraction of trace elements. *Spectrochim Acta Part B*, 58: 1177–1233.
- Chen C T, Chen Y C, 2005. Fe₃O₄/TiO₂ core/shell nanoparticles as affinity probes for the analysis of phosphopeptides using tio₂ surface-assisted laser desorption/ionization mass spectrometry. *Analytical Chemistry*, 77: 5912–5919.
- Decision No 2455/2001/EC of the European Parliament and of the Council of 20 November 2001 establishing the list of priority substances in the field of water policy and amending Directive 2000/60/EC, (15 December) 2001. *Official Journal of the European Communities*, L331: 1–5.
- Directive 2000/60/EC of the European Parliament and of the Council establishing a framework for Community action in the field of water policy. *CELEX-EUR official Journal L327*, 22 December 2000. 1–72.
- Diebold U, 2003. The surface science of titanium dioxide. *Surface Science Reports*, 48: 53–229.
- Edisson M J, Marco A S, Gustavo T M, Bojan A M, Paula M J, Antonio S A, 2006. A study on the structure and thermal stability of titanate nanotubes as a function of sodium content. *Solid State Sciences*, 8: 888–900.
- Ikeguchi Y, Nakamura H, 1998. A novel method for the on-line

- room-temperature hydrolysis of hydrophobic organic phosphates using a cooperative action of sodium dodecyl sulfate, acid and UV-irradiation. *Analytical Sciences*, 14: 815–817.
- Ikeguchi Y, Nakamura H, 1999. Fluorometric determination of phospholipids by high-performance liquid chromatography with postcolumn on-line hydrolysis under UV-irradiation, phosphomolybdic acid and thiamine-thiochrome reactions. *Analytical Sciences*, 15: 229–232.
- Ikeguchi Y, Nakamura H, 2000. Selective enrichment of phospholipids by titania. *Analytical Sciences*, 16: 541–543.
- Jung J H, Kobayashi H, van Bommel K J C, Shinkai S, Shimizu T, 2002. Creation of novel helical ribbon and double-layered nanotube TiO₂ structures using an organogel template. *Chemistry of Materials*, 14: 1445–1447.
- Kasuga T, 2006. Formation of titanium oxide nanotubes using chemical treatments and their characteristic properties. *Thin Solid Films*, 496: 141–145.
- Kawahara M, Nakamura H, Nakajima T, 1989. Group separation of ribonucleosides and deoxyribonucleosides on a new ceramic titania column. *Analytical Sciences*, 5: 763–764.
- Kochkar H, Lakhthar N, Berhault G, Bausach M, Ghorbel A, 2009. Optimization of the alkaline hydrothermal route to titanate nanotubes by a doehlert matrix experience design. *Journal of Physical Chemistry C*, 113: 1672–1679.
- Li K, Christensen E R, Van Camp R P, Imamoglu I, 2001. PAHs in dated sediments of ashtabula river, Ohio, USA. *Environmental Science and Technology*, 35: 2896–2902.
- Li S Q, Hu B, Jiang Z C, Liang P, Li X, Xia L B, 2004. Selective separation of La³⁺ and lanthanum organic complexes with nanometer-sized titanium dioxide and their detection by using fluorination-assisted electrothermal vaporization ICP-AES with *in-situ* matrix removal. *Environmental Sciences and Technology*, 38: 2248–2251.
- Li S X, Deng N S, 2002. Separation and preconcentration of Se(IV)/Se(VI) species by selective adsorption onto nanometer-sized titanium dioxide and determination by graphite furnace atomic absorption spectrometry. *Analytical and Bioanalytical Chemistry*, 374: 1341–1345.
- Liang P, Hu B, Jiang Z C, 2001. Nanometer-sized titanium dioxide micro-column on-line preconcentration of La, Y, Yb, Eu, Dy and their determination by inductively coupled plasma atomic emission spectrometry. *Journal of Analytical Atomic Spectrometry*, 16: 863–866.
- Liu A H, Wie M D, Honma I, Zhou H S, 2005. Direct electrochemistry of myoglobin in titanate nanotubes film. *Analytical Chemistry*, 77: 8068–8074.
- Liu Z J, Zhang Q, Qin L C, 2007. Reduction in the electronic band gap of titanium oxide nanotubes. *Solid State Communication*, 141: 168–171.
- Matsuda H, Nakamura H, Nakajima T, 1991. New ceramic titania: selective adsorbent for organic phosphates. *Analytical Sciences*, 7: 813–814.
- Mor G K, Varghese O K, Paulose M, Shankar K, Grimes C A, 2006. A review on highly ordered, vertically oriented TiO₂ nanotube arrays: fabrication, material properties, and solar energy applications. *Solar Energy Materials and Solar Cells*, 90: 2011–2075.
- Nawrocki J, Dunlap C, McCormick A, Carr P W, 2004. Part I. Chromatography using ultra-stable metal oxide-based stationary phases for HPLC. *Journal of Chromatography A*, 1028: 1–30.
- Oleszczuk P, Stanisław B, 2004. Application of solid-phase extraction to determination of polycyclic aromatic hydrocarbons in sewage sludge extracts. *Journal of Hazardous Materials*, 113: 237–245.
- Pinkse M H, Uitto P M, Hilhorst M J, Ooms B, Heck A J R, 2004. Selective isolation at the femtomole level of phosphopeptides from proteolytic digests using 2D-NanoLC-ESI-MS/MS and titanium oxide precolumns. *Analytical Chemistry*, 76: 3935–3943.
- Poster D L, Schantz M M, Sander L C, Wise S A, 2006. Analysis of polycyclic aromatic hydrocarbons (PAHs) in environmental samples: a critical review of gas chromatographic (GC) methods. *Analytical and Bioanalytical Chemistry*, 386: 859–881.
- Sano A, Nakamura H, 2004. Chemo-affinity of titania for the column-switching HPLC analysis of phosphopeptides. *Analytical Chemistry*, 20: 565–566.
- Sano A, Nakamura H, 2004. Titania as a chemo-affinity support for the column-switching HPLC analysis of phosphopeptides: application to the characterization of phosphorylation sites in proteins by combination with protease digestion and electrospray ionization mass spectrometry. *Analytical Chemistry*, 20: 861–864.
- Vassileva E, Proinova I, Hadjiivanov K, 1996. Solid-phase extraction of heavy metal ions on a high surface area titanium dioxide (anatase). *Analyst*, 121: 607–612.
- Yang J J, Jin Z S, Wang X D, Li W, Zhang J W, Zhang S L, et al., 2003. Study on composition, structure and formation process of nanotube Na₂Ti₂O₄(OH)₂. *Dalton Transactions*, 20: 3898–3901.
- Wang W D, Huang Y M, Shu W Q, Cao J, 2007. Multiwalled carbon nanotubes as adsorbents of solid-phase extraction for determination of polycyclic aromatic hydrocarbons in environmental waters coupled with high-performance liquid chromatography. *Journal of Chromatography A*, 1173: 27–36.
- Yang K, Wang X L, Zhu L Z, Xing B S, 2006a. Competitive sorption of pyrene, phenanthrene, and naphthalene on multiwalled carbon nanotubes. *Environmental Sciences and Technology*, 40: 5804–5810.
- Yang K, Xing B S, 2006. Desorption of polycyclic aromatic hydrocarbons from carbon nanomaterials in water. *Environmental Pollution*, 145: 529–537.
- Yang K, Zhu L Z, Xing B S, 2006b. Adsorption of polycyclic aromatic hydrocarbons by carbon nanomaterials. *Environmental Science and Technology*, 40: 1855–1861.
- Zhang L, Ishi D, Shitou K, Morita Y, Isozaki A, 2005. Simultaneous multi-element analysis of total As, Se and Sb on titanium dioxide by slurry sampling-graphite furnace atomic absorption spectrometry. *Talanta*, 68(2): 336–342.
- Zhou Q X, Ding Y J, Xiao J P, Liu G G, Guo X Y, 2007. Investigation of the feasibility of TiO₂ nanotubes for the enrichment of DDT and its metabolites at trace levels in environmental water samples. *Journal of Chromatography A*, 1147: 10–16.